

Method Extension of CIPAC 578 in Flumioxazin SC

Test Facility: Name: Shandong Binnong Technology Co., Ltd.
Address: No.518, Yongxin Road, Binbei Town, Binzhou, Shandong, China
Tel: 86-543-5087891
Fax: 86-543-5087891

Sponsor: Name: Shandong Binnong Technology Co., Ltd.
Address: No.518, Yongxin Road, Binbei Town, Binzhou, Shandong, China
Tel: 86-543-3363985
Fax: 86-543-3163179

Chief Analyzer: Name: Ms. Sun Jing
Address: No.518, Yongxin Road, Binbei Town, Binzhou, Shandong, China
Tel: 86-543-5087153
Fax: 86-543-5087891

Test Guideline: CIPAC No. 3807, CIPAC 578

Content

Title Page.....	1
Content	2
STATEMENT	3
1. Summary.....	4
2. Introduction	5
3. Material	5
3.1 Specification of test item	5
3.2 Specification of reference item.....	5
3.3 Storage conditions	5
4. Experimental Procedure.....	6
4.1 Reagents.....	6
4.2 Equipment.....	6
4.3 Analytical condition.....	6
4.4 Specificity test	6
4.5 Linearity check	7
5. Result and Conclusion	7
5.1 Specificity test results.....	7
5.2 Linearity check results.....	8
6. Amendment and deviation.....	9
7. Reference	9
8. Appendix	9
APPENDIX A: COPY OF CHROMATOGRAM.....	10
FIGURE 1: CHROMATOGRAM OF ACETONITRILE, (SOLVENT).....	10
FIGURE 2: CHROMATOGRAM OF BLANK FORMULATION	11
FIGURE 3: CHROMATOGRAM OF REFERENCE ITEM.....	12
FIGURE 4: CHROMATOGRAM OF TEST ITEM.....	13
FIGURE 5: PEAK PURITY OF REFERENCE ITEM	14
FIGURE 6: PEAK PURITY OF TEST ITEM	15
FIGURE 7: LINEARITY CHECK FOR LIN-1, injection 1	16
FIGURE 8: LINEARITY CHECK FOR LIN-1, injection 2	17
FIGURE 9: LINEARITY CHECK FOR LIN-2, injection 1	18
FIGURE 10: LINEARITY CHECK FOR LIN-2, injection 2	19
FIGURE 11: LINEARITY CHECK FOR LIN-3, injection 1.....	20
FIGURE 12: LINEARITY CHECK FOR LIN-3, injection 2	21
APPENDIX B: CERTIFICATE OF ANALYSIS FOR TEST ITEM	22
APPENDIX C: CERTIFICATE OF ANALYSIS FOR REFERENCE ITEM	23

STATEMENT

Test substance: Flumioxazin SC

Study Title: Method Extension of CIPAC 578 in Flumioxazin SC

Study No.: BNS20220052

This study was designed and performed by QC Center of Shandong Binnong Technology Co., Ltd. To the best of our knowledge, there were no deviations from the study protocol affecting the quality or integrity of the study.

This report accurately reflects the raw data and accurately describes the methods and standard operation procedures used in this study.

Chief Analyzer: Sun Jing

Signature:



Date: 2022-06-08

Shandong Binnong Technology Co., Ltd.

1. Summary

For Flumioxazin SC, there is no CIPAC method available. To determine whether the method (CIPAC 578) can be applied for the new formulation of Flumioxazin SC, a specificity test was performed according to the procedure of the extension of the scope of methods. The results are summarized in the following Table 1 and Table 2.

Table 1 The specificity test results

Solution tested	Conclusion
Acetonitrile (Solvent)	No interferences were detected at the retention time of the active ingredient.
Blank formulation	
Test item solution	
Reference item solution	

Table 2 Peak purity analysis results

Sample solution name	Purity threshold	Purity factor
Test item solution	990.000	999.944
Reference item solution	990.000	999.690

According to the specificity test and peak purity analysis results, the method (CIPAC 578) was considered specific applied for the Flumioxazin SC.

And the concentration of flumioxazin analyte is inside the acceptability range covered by the sample, so the method (CIPAC 578) can be applied for Flumioxazin SC.


2. Introduction

The objective of the study is to evaluate whether the method (CIPAC 578) is suitable for the determination of flumioxazin in SC formulation.

3. Material

3.1 Specification of test item

The related information and analytical identification provided by the sponsor was the responsibility of the sponsor. The details of the test items are given as follow:

Product name	Flumioxazin SC
Molecular formula of AI	C ₁₉ H ₁₅ FN ₂ O ₄
Molecular weight of AI	354.3 g/mol
Structure formula of AI	
Chemical name (IUPAC) of AI	N-(7-fluoro-3,4-dihydro-3-oxo-4-prop-2-ynyl-2H-1,4-benzoxazin-6-yl) cyclohex-1-ene-1,2-dicarboxamide
CAS No. of AI	103361-09-7
Physical state	Off-white liquid
Batch No.	202206007
Active ingredient, g/l (w/v)	482
Density, (g/cm ³)	1.174
Manufacture date	June 02, 2022
Retest date	June 02, 2024
Storage condition	Store in original container, in a well-ventilated, cool, dry, secure area.
Manufacturer	Shandong Binnong Technology Co., Ltd.
Address of manufacturer	No.518, Yongxin Road, Binbei Town, Binzhou, Shandong, China

Certificate of analysis for test item are presented in **Appendix B**.

3.2 Specification of reference item

Product Name	Flumioxazin
CAS Number	103361-09-7
Lot No.	G140220
Purity	99.47%
Certified date	May 26, 2017
Expiry Date	February 16, 2023
Storage Condition	20±4 °C
Manufacturer	Dr. Ehrenstorfer

Certificate of analysis for reference item are presented in **Appendix C**.

3.3 Storage conditions

The test item was stored at 20±10 °C in Test Substance Control Office of BNS QC Center. The

reference item was stored at 20±4°C in refrigerator in BNS QC Center. They are treated according to relevant SOP for reception, storage and distribution.

4. Experimental Procedure

4.1 Reagents

Flumioxazin reference item, purity 99.47%, Lot No.: G140220, supplied by Dr. Ehrenstorfer.

Acetonitrile, HPLC grade, Lot No.: I0972907839, supplied by Merck KGaA, Germany.

Ultrapure water, resistivity: ≥10 MΩ·cm, prepared by ultrapure water machine.

4.2 Equipment

Agilent 1260 Infinity II LC system, with DAD detector, supplied by Agilent Technologies Pte., Ltd, USA;

Electronic balance, type: XSE205DU, supplied by Mettler-Toledo Instrument Co., Ltd, Switzerland.

Ultrapure water machine, type: UPR- II -20L, supplied by ULUPURE Ultrapure Technology Co., Ltd, China.

Ultrasonic cleaner, type: AS-3120, supplied by Tianjin Automatic Science Instrument Co., Ltd, China.

Volumetric flask, 100 ml, supplied by Tianjin Glass Instrument Manufacturing Co., Ltd, China.

Nylon syringe filters, 0.22 μm, supplied by Tianjin Heshi Science and Technology Development Ltd., China.

Disposable syringe, 5 mL, supplied by Henan Shu Guang Jian Shi Medical Apparatus and Instruments Co., Ltd., China.

4.3 Analytical condition

Detector:	DAD		
Wavelength:	288 nm		
Column:	Phenomenex Gemini (250mm x 4.6mm x 5μm)		
Column temperature:	40°C		
Injection volume:	10.0 μl		
Mobile phase:	Solvent A: Ultrapure Water Solvent B: Acetonitrile		
Stop time:	15 min		
Post time	0 min		
Time (min)	Flow (mL/min)	A (%)	B (%)
0	1.000	50	50

4.4 Specificity test

The specificity of the method was evaluated by injecting Acetonitrile (solvent used for solution preparation), blank formulation, test item solution and reference item solutions to check for any interfering peak at the retention time of the peak of interest.

Blank formulation solution preparation: 71.27mg of blank formulation was weighed into a 100 mL volumetric flask. About 80 mL Acetonitrile was added into flask and the flask was shaken to dissolve. The flask was placed in ultrasonic bath for 10 min, then cool to ambient temperature. The solution was made up to the mark using Acetonitrile and mixed well.

Test item solution preparation: 123.72mg of test item was weighed into a 100 mL volumetric flask. About 80 mL Acetonitrile was added into flask and the flask was shaken to dissolve. The flask was placed in ultrasonic bath for 10 min, then cool to ambient temperature. The solution was made up to the mark using Acetonitrile and mixed well.

Reference item solution preparation: 50.63mg of reference item was weighed into a 100 mL volumetric flask. About 80 mL Acetonitrile was added into flask and the flask was shaken to dissolve. The flask was placed in ultrasonic bath for 10 min, then cool to ambient temperature. The solution was made up to the mark using Acetonitrile and mixed well.

All the solutions were filtered through a 0.22 µm filter prior to analysis.

And inject at least 2 portions of Reference item solutions for system equilibration before performing the specificity test.

4.5 Linearity check

Check the linearity of the detector response by injecting 10 µl of solutions with flumioxazin concentrations 0.5, 1 and 2 times that of the Reference item solution to determine whether the concentration of the flumioxazin is inside the acceptability range covered by the samples applied in the method (CIPAC 578).

Lin-1: 25.09mg of reference item was weighed into a 100 mL volumetric flask. About 80 mL Acetonitrile was added into flask and the flask was shaken to dissolve. The flask was placed in ultrasonic bath for 10 min, then cool to ambient temperature. The solution was made up to the mark using Acetonitrile and mixed well.

Lin-2: 50.03mg of reference item was weighed into a 100 mL volumetric flask. About 80 mL Acetonitrile was added into flask and the flask was shaken to dissolve. The flask was placed in ultrasonic bath for 10 min, then cool to ambient temperature. The solution was made up to the mark using Acetonitrile and mixed well.

Lin-3: 100.19mg of reference item was weighed into a 100 mL volumetric flask. About 80 mL Acetonitrile was added into flask and the flask was shaken to dissolve. The flask was placed in ultrasonic bath for 10 min, then cool to ambient temperature. The solution was made up to the mark using Acetonitrile and mixed well.

All the solutions were filtered through a 0.22 µm filter prior to analysis.

5. Result and Conclusion

5.1 Specificity test results

Table 1 Specificity of Flumioxazin SC

Solution tested	Conclusion
Acetonitrile (Solvent)	No interferences were detected at the retention time of the active ingredient.
Blank formulation	
Test item solution	
Reference item solution	

The specificity relevant chromatograms, are listed in Appendix A, figure 1-4.

Peak purity analysis was performed using a DAD detector to detect the presence of any other substance co-eluting with the analyte peak. The peak purity factor of the sample solutions was greater than the peak purity threshold, indicating that there was no interference. That shows a

good peak purity.

Table 2 Peak purity of Flumioxazin in the method

Sample solution name	Purity threshold	Purity factor
Test item solution	990.000	999.944
Reference item solution	990.000	999.690

The peak purity analysis related chromatograms, are listed in Appendix A, figure 5-6.


From the above specificity test, the method (CIPAC 578) used for flumioxazin SC formulation is specific.

5.2 Linearity check results

From the CIPAC guideline “EXTENSION OF THE SCOPE OF METHODS”, the acceptability range is from 200 % to 50 % of the concentration of an analyte in a sample studied.

The 3 concentrations (0.5, 1, 2 times) of the Flumioxazin Reference item solution, were injected with duplicate for each. The line was generated with slope, intercept and correlation coefficient data.

The linearity chromatograms, are listed in Appendix A, figure 7-12.

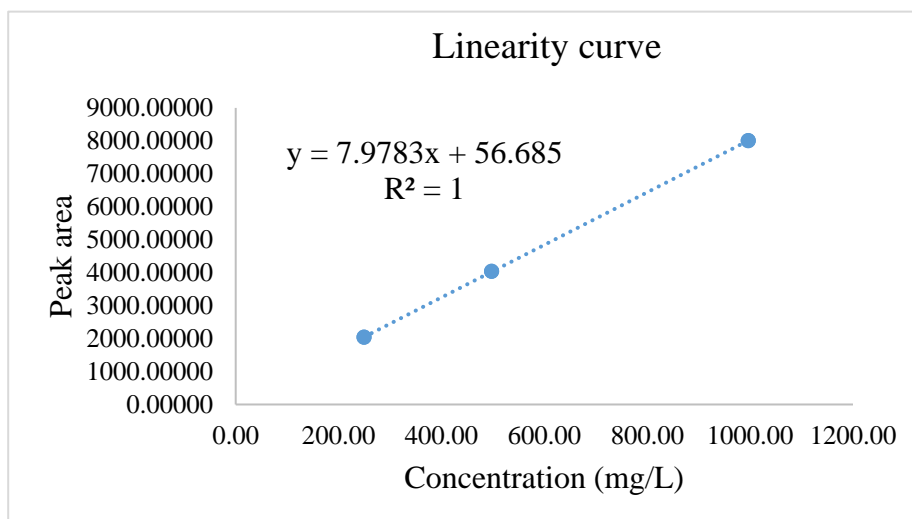

The correlation coefficient (r) is > 0.99 . over the range (200% ~ 50% of the nominal).

The test item solution injected for specificity test with peak area 4099.29883, is in the range of the linearity concentration.

Table 3 Peak area of Flumioxazin reference and test item solutions

Sample solution name	Lin-1	Lin-2	Lin-3
Average peak area for 2 injections	2039.49677	4039.52466	8003.60865
Peak area of Test item solution for specificity	4099.29883		
Peak area of Reference item solution for specificity	4069.88550		

From the table 3, the peak area of Test item solution for specificity is nearly with the peak area of Lin-2, which indicate the concentration of analyte in test item solution for specificity is nearly with the concentration of analyte in Lin-2(100% of nominal analyte concentration).

The other hand, the sample content is 41.2% (w/w) $(482/1.174/1000 * 100\% = 41.1\%$, indicated

in sponsor COA), which contains the analyte flumioxazin concentration as follows: $123.72\text{mg} / 100\text{ml} * 1000 * 41.1\% = 508.5\text{mg/l}$, and in the method (CIPAC 578), the nominal concentration of flumioxazin used as $(50\text{mg} / 100\text{ml} = 500\text{mg/l})$, so, the acceptability range is $508.5/500 * 100\% = 101.7\%$, which is in the acceptable range between 200% and 50%.

6. Amendment and deviation

The test is focus on the extension of the flumioxazin CIPAC method to flumioxazin SC formulation. The specificity test was conducted completely follow the CIPAC method without any change.

7. Reference

- (1) CIPAC No.3807 Guidelines on method validation to be performed in support of analytical methods for agrochemical formulations.
- (2) CIPAC Method (578/TC/M/3, 578/WP/M/3).
- (3) CIPAC guideline 'Extension of the scope of methods'.

8. Appendix

APPENDIX A: COPY OF CHROMATOGRAM


APPENDIX B: CERTIFICATE OF ANALYSIS FOR TEST ITEM

APPENDIX C: CERTIFICATE OF ANALYSIS FOR REFERENCE ITEM

APPENDIX A: COPY OF CHROMATOGRAM

Data File D:\HPLC\DA...LUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\004-P2-A4-Acetonitrile.D
Sample Name: Acetonitrile

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    4
Acq. Instrument : LC 1260 DAD                 Location  : P2-A-04
Injection Date  : 6/7/2022 6:05:51 PM        Inj       :    1
                                           Inj Volume: 10.000 µl
Acq. Method     : D:\HPLC\Data\Flumioxazin\Flumioxazin 2022-06-07 17-17-09\flumioxazin.M
Last changed    : 11/17/2021 8:30:46 AM by SYSTEM
Analysis Method : D:\HPLC\METHOD\FLUMIOXAZIN\flumioxazin-1.M
Last changed    : 6/8/2022 4:13:11 PM by SYSTEM
=====
```

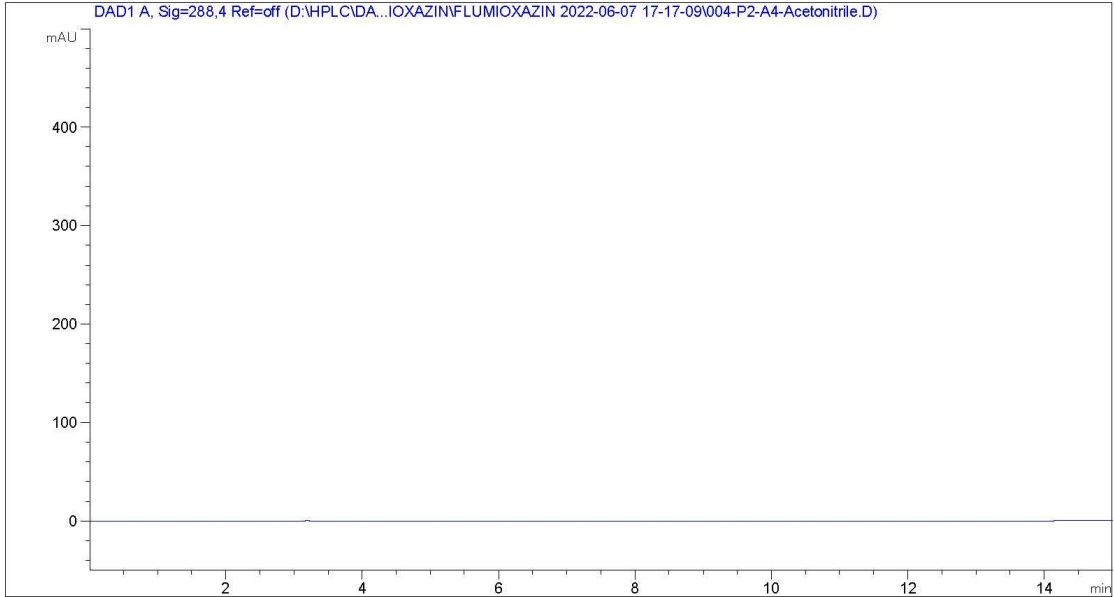

```
=====
                          Area Percent Report
=====
```

```
Sorted By           :      Signal
Multiplier          :      1.0000
Dilution            :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```


No peaks found

```
=====
*** End of Report ***
=====
```

FIGURE 1: CHROMATOGRAM OF ACETONITRILE, SOLVENT)

Data File D:\HPLC\DATA\FLUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\005-P2-A5-Blank-SC.D
Sample Name: Blank-SC

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    5
Acq. Instrument : LC 1260 DAD                 Location  : P2-A-05
Injection Date  : 6/7/2022 6:21:47 PM        Inj       :    1
                                           Inj Volume: 10.000 µl
Acq. Method     : D:\HPLC\Data\Flumioxazin\Flumioxazin 2022-06-07 17-17-09\Flumioxazin.M
Last changed    : 11/17/2021 8:30:46 AM by SYSTEM
Analysis Method : D:\HPLC\METHOD\FLUMIOXAZIN\flumioxazin-1.M
Last changed    : 6/8/2022 4:13:11 PM by SYSTEM
=====
```

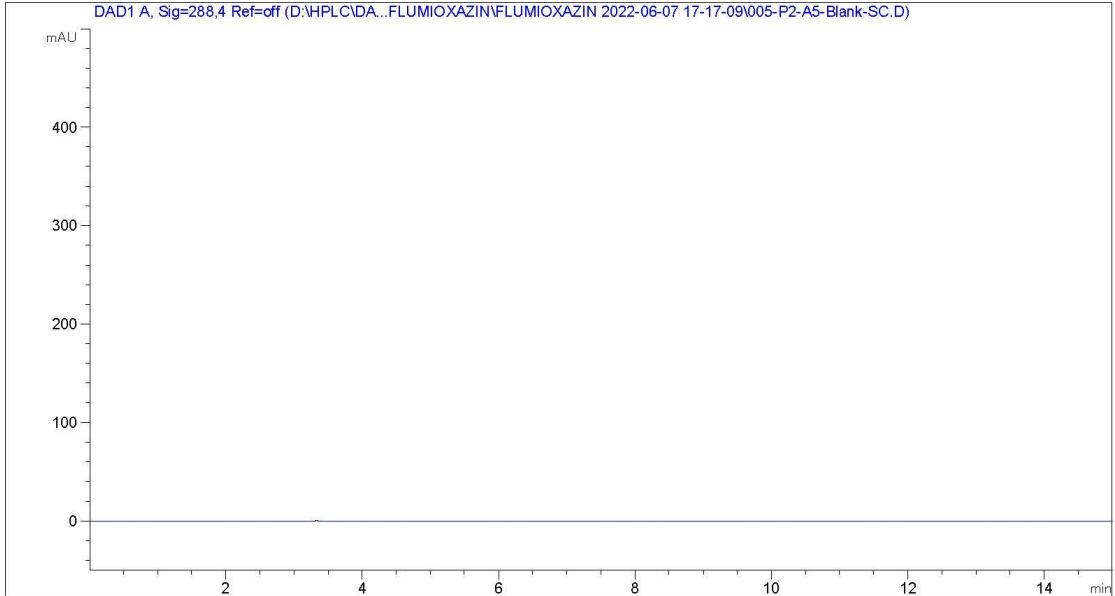

```
=====
                          Area Percent Report
=====
```

```
Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found
```

```
=====
*** End of Report ***
=====
```


FIGURE 2: CHROMATOGRAM OF BLANK FORMULATION

Data File D:\HPLC\DATA\FLUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\007-P2-A7-Sample-SC.D
 Sample Name: Sample-SC

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    7
Acq. Instrument : LC 1260 DAD                 Location  : P2-A-07
Injection Date  : 6/7/2022 6:53:40 PM        Inj       :    1
                                           Inj Volume: 10.000 µl

Acq. Method     : D:\HPLC\Data\Flumioxazin\Flumioxazin 2022-06-07 17-17-09\flumioxazin.M
Last changed    : 11/17/2021 8:30:46 AM by SYSTEM
Analysis Method : D:\HPLC\METHOD\FLUMIOXAZIN\flumioxazin-1.M
Last changed    : 6/8/2022 4:13:11 PM by SYSTEM
  
```

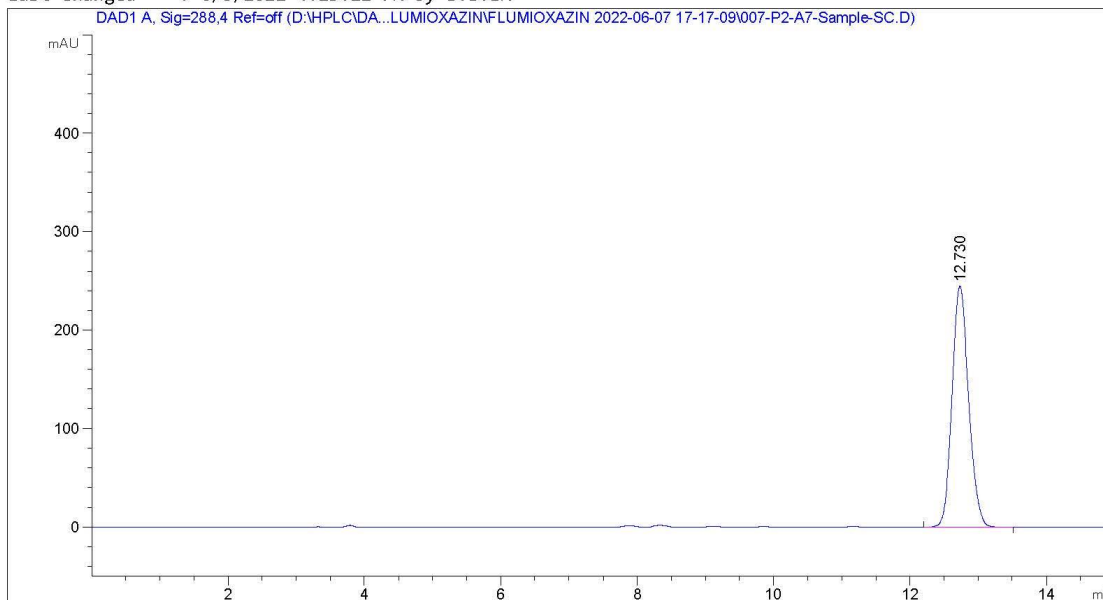

=====
 Area Percent Report
 =====

```

Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: DAD1 A, Sig=288,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	12.730	BB	0.2577	4099.29883	244.41884	100.0000

Totals : 4099.29883 244.41884



=====
 *** End of Report ***

FIGURE 4: CHROMATOGRAM OF TEST ITEM

Data File D:\HPLC\DA...MIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\006-P2-A6-Reference item.D
Sample Name: Reference item

Purity results peak 1 at 12.722 min.

Signal DAD1 A, Sig=288,4 Ref=off (D:\HPLC\DA...XAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\006-P2-

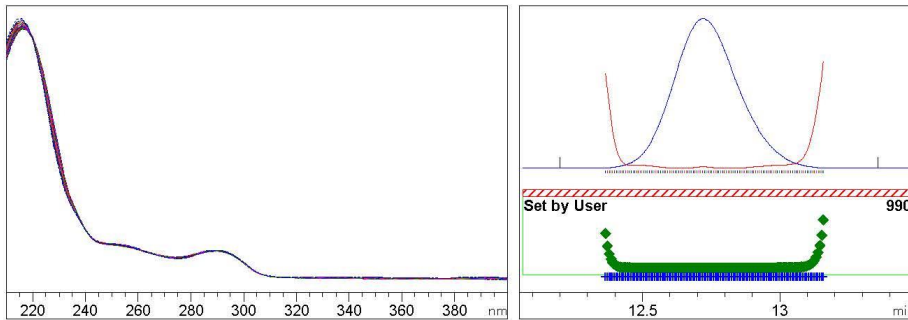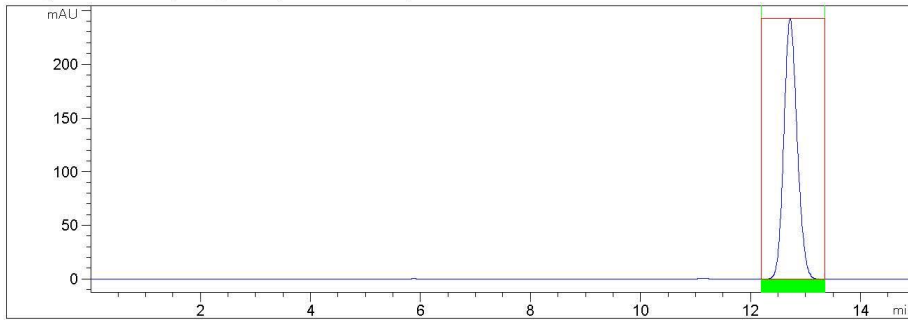

-> The purity factor is within the threshold limit. <-

Purity factor : 999.690 (120 of 120 spectra are within the threshold limit.)
Threshold : 990.000 (Set by user)
Reference : Nearest baseline spectrum (stored) (0.005)
Spectra : 120 (Selection automatic, All)
Warning : Spectral absorbances > 1000 mAU (see help for more information)




*** End of Report ***

FIGURE 5: PEAK PURITY OF REFERENCE ITEM

Data File D:\HPLC\DATA\FLUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\007-P2-A7-Sample-SC.D
 Sample Name: Sample-SC

Purity results peak 1 at 12.730 min.

Signal DAD1 A, Sig=288,4 Ref=off (D:\HPLC\DA...LUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\007-P2-A7-Sample-SC.D)

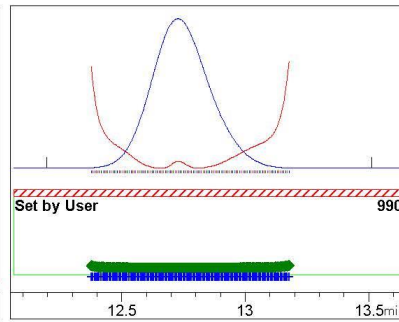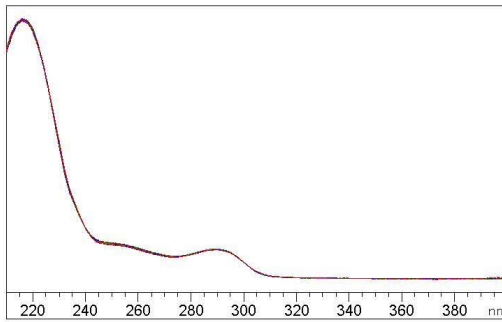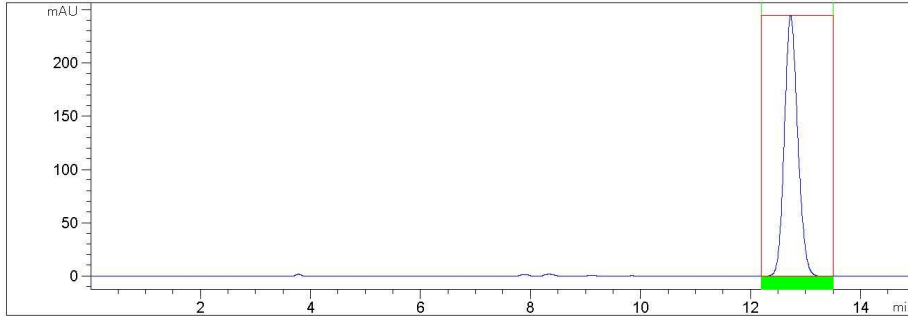

-> The purity factor is within the threshold limit. <-

Purity factor : 999.944 (121 of 121 spectra are within the threshold limit.)
 Threshold : 990.000 (Set by user)
 Reference : Nearest baseline spectrum (stored) (0.003)
 Spectra : 121 (Selection automatic, All)
 Warning : Spectral absorbances > 1000 mAU (see help for more information)

*** End of Report ***


FIGURE 6: PEAK PURITY OF TEST ITEM

Data File D:\HPLC\DATA\FLUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\008-P2-A1-Lin-1.D
 Sample Name: Lin-1

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    8
Acq. Instrument : LC 1260 DAD                 Location  : P2-A-01
Injection Date  : 6/7/2022 7:09:35 PM        Inj       :    1
                                           Inj Volume: 10.000 µl

Acq. Method     : D:\HPLC\Data\Flumioxazin\Flumioxazin 2022-06-07 17-17-09\Flumioxazin.M
Last changed    : 11/17/2021 8:30:46 AM by SYSTEM
Analysis Method : D:\HPLC\METHOD\FLUMIOXAZIN\flumioxazin 1.M
Last changed    : 6/8/2022 9:14:04 AM by SYSTEM
  
```

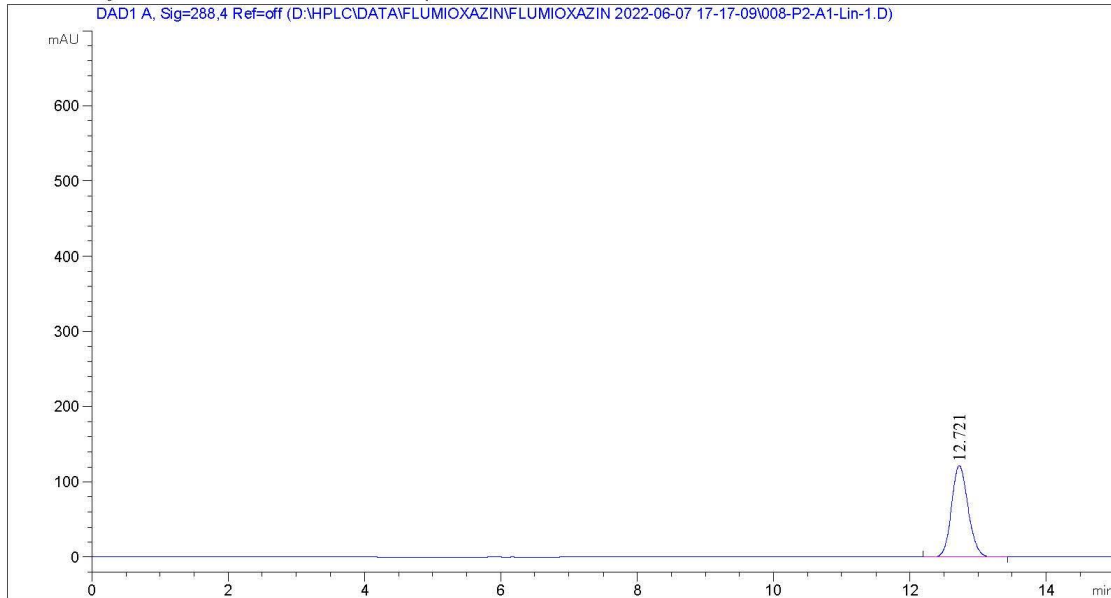

Area Percent Report

```

=====
Sorted By      : Signal
Calib. Data Modified : 6/8/2022 8:32:43 AM
Multiplier     : 1.0000
Dilution       : 1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: DAD1 A, Sig=288,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	12.721	BB	0.2579	2040.12903	100.0000	Flumioxazin

Totals : 2040.12903


*** End of Report ***

FIGURE 7: LINEARITY CHECK FOR LIN-1, injection 1

Data File D:\HPLC\DATA\FLUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\009-P2-A1-Lin-1.D
 Sample Name: Lin-1

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    9
Acq. Instrument : LC 1260 DAD                 Location  : P2-A-01
Injection Date  : 6/7/2022 7:25:31 PM        Inj       :    2
                                           Inj Volume: 10.000 µl
Acq. Method     : D:\HPLC\Data\Flumioxazin\Flumioxazin 2022-06-07 17-17-09\Flumioxazin.M
Last changed    : 11/17/2021 8:30:46 AM by SYSTEM
Analysis Method : D:\HPLC\METHOD\FLUMIOXAZIN\flumioxazin 1.M
Last changed    : 6/8/2022 9:14:04 AM by SYSTEM
  
```

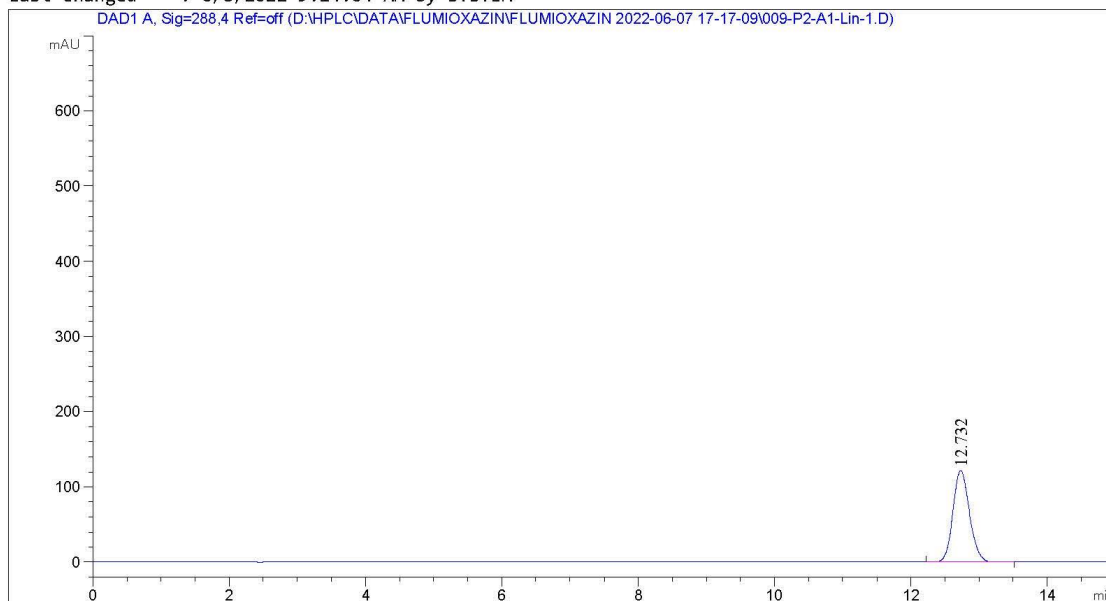

=====
 Area Percent Report
 =====

```

Sorted By      :      Signal
Calib. Data Modified : 6/8/2022 8:32:43 AM
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: DAD1 A, Sig=288,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	12.732	BB	0.2575	2038.86450	100.0000	Flumioxazin

Totals : 2038.86450

=====
 *** End of Report ***


FIGURE 8: LINEARITY CHECK FOR LIN-1, injection 2

Data File D:\HPLC\DATA\FLUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\010-P2-A2-Lin-2.D
 Sample Name: Lin-2

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :   10
Acq. Instrument : LC 1260 DAD                 Location  : P2-A-02
Injection Date  : 6/7/2022 7:41:26 PM        Inj       :    1
                                           Inj Volume: 10.000 µl

Acq. Method     : D:\HPLC\Data\Flumioxazin\Flumioxazin 2022-06-07 17-17-09\Flumioxazin.M
Last changed    : 11/17/2021 8:30:46 AM by SYSTEM
Analysis Method : D:\HPLC\METHOD\FLUMIOXAZIN\flumioxazin 1.M
Last changed    : 6/8/2022 9:14:04 AM by SYSTEM
  
```

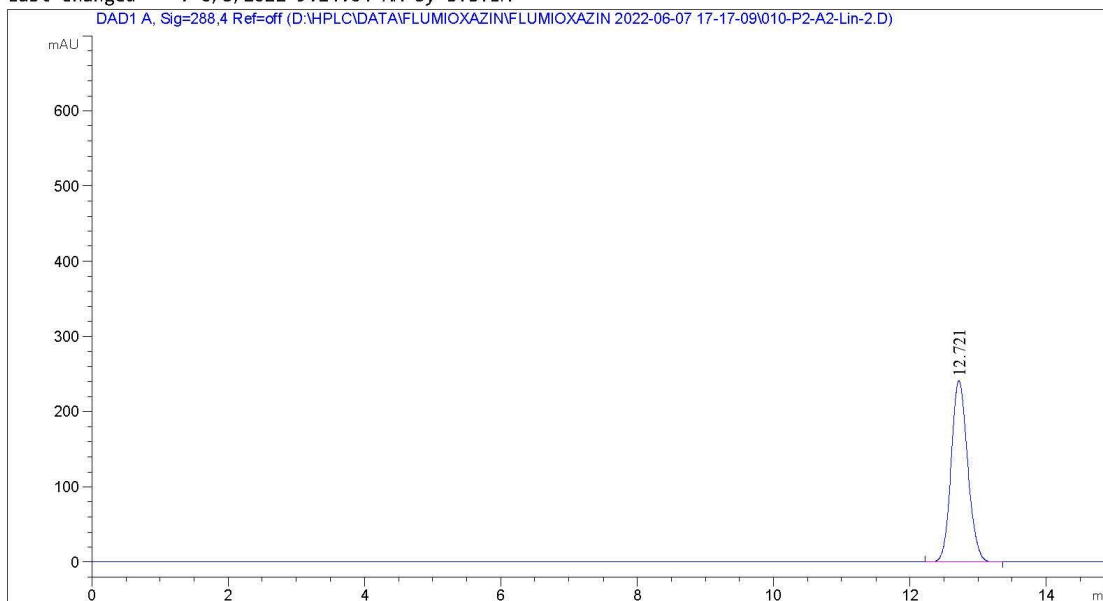

Area Percent Report

```

=====
Sorted By      :      Signal
Calib. Data Modified : 6/8/2022 8:32:43 AM
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: DAD1 A, Sig=288,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	12.721	BB	0.2577	4038.73486	100.0000	Flumioxazin

Totals : 4038.73486

*** End of Report ***


FIGURE 9: LINEARITY CHECK FOR LIN-2, injection 1

Data File D:\HPLC\DATA\FLUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\012-P2-A3-Lin-3.D
 Sample Name: Lin-3

```

=====
Acq. Operator   : SYSTEM                      Seq. Line : 12
Acq. Instrument : LC 1260 DAD                 Location  : P2-A-03
Injection Date  : 6/7/2022 8:13:19 PM        Inj       : 1
                                                Inj Volume: 10.000 µl

Acq. Method     : D:\HPLC\Data\Flumioxazin\Flumioxazin 2022-06-07 17-17-09\Flumioxazin.M
Last changed    : 11/17/2021 8:30:46 AM by SYSTEM
Analysis Method : D:\HPLC\METHOD\FLUMIOXAZIN\flumioxazin 1.M
Last changed    : 6/8/2022 9:14:04 AM by SYSTEM
  
```

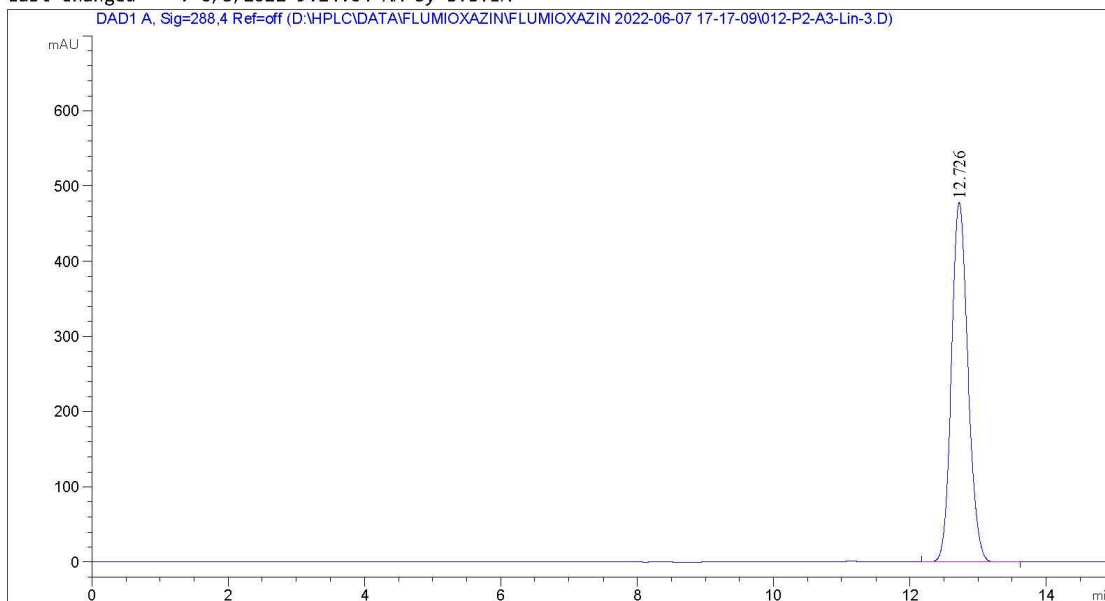

=====
 Area Percent Report
 =====

```

Sorted By      : Signal
Calib. Data Modified : 6/8/2022 8:32:43 AM
Multiplier     : 1.0000
Dilution       : 1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: DAD1 A, Sig=288,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	12.726	BB	0.2573	8005.55225	100.0000	Flumioxazin

Totals : 8005.55225

=====
 *** End of Report ***

FIGURE 11: LINEARITY CHECK FOR LIN-3, injection 1


Data File D:\HPLC\DATA\FLUMIOXAZIN\FLUMIOXAZIN 2022-06-07 17-17-09\013-P2-A3-Lin-3.D

Sample Name: Lin-3

```

=====
Acq. Operator   : SYSTEM                      Seq. Line : 13
Acq. Instrument : LC 1260 DAD                 Location  : P2-A-03
Injection Date  : 6/7/2022 8:29:14 PM        Inj       : 2
                                           Inj Volume: 10.000 µl

Acq. Method     : D:\HPLC\Data\Flumioxazin\Flumioxazin 2022-06-07 17-17-09\Flumioxazin.M
Last changed    : 11/17/2021 8:30:46 AM by SYSTEM
Analysis Method : D:\HPLC\METHOD\FLUMIOXAZIN\flumioxazin 1.M
Last changed    : 6/8/2022 9:14:04 AM by SYSTEM
    
```

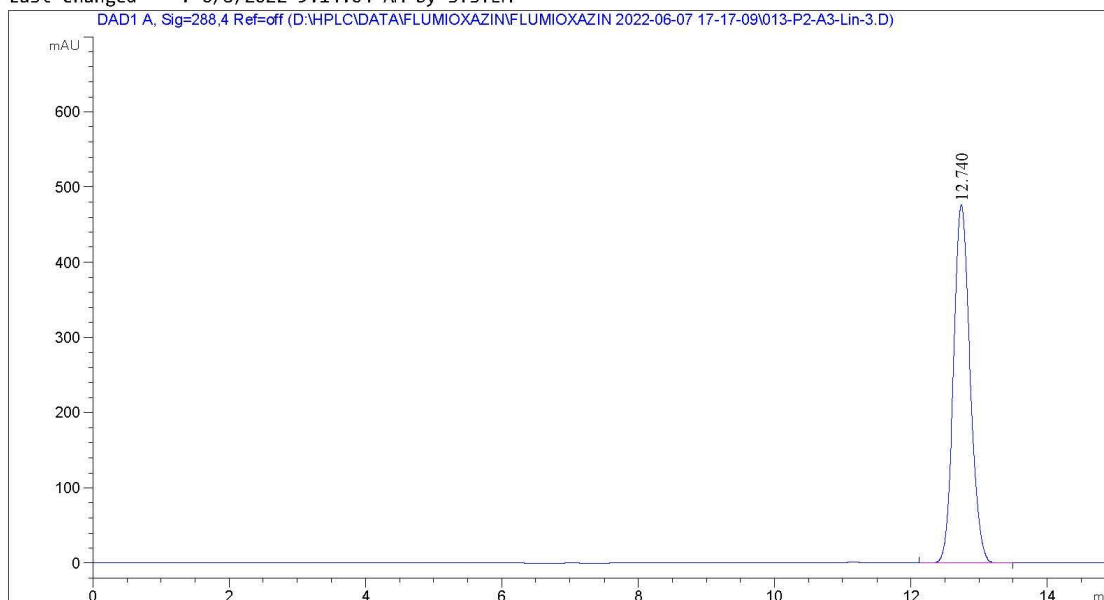

=====
Area Percent Report
 =====

```

Sorted By      : Signal
Calib. Data Modified : 6/8/2022 8:32:43 AM
Multiplier     : 1.0000
Dilution       : 1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: DAD1 A, Sig=288,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	12.740	BB	0.2580	8001.66504	100.0000	Flumioxazin

Totals : 8001.66504

=====
 *** End of Report ***

FIGURE 12: LINEARITY CHECK FOR LIN-3, injection 2

APPENDIX B: CERTIFICATE OF ANALYSIS FOR TEST ITEM

CERTIFICATE OF ANALYSIS

Product Name	Flumioxazin SC		
Manufacture Date	June 02, 2022	Test Date	June 02, 2022
Batch No.	202206007	Expiry Date	June 02, 2024
Test Result & Conclusion			
Analysis Items	Specification	Test results	
Appearance	Off-white liquid	Off-white liquid	
Active ingredient, g/l (w/v)	≥ 480	482	
Density (g/cm ³)	1.174		
Storage condition	Store in original container, in a well-ventilated, cool, dry, secure area.		
All the items are qualified for use and transport			
Report Date: June 02, 2022			

Chief Analyzer: Sun Jing

Examiner: Song Shuyan

Inspector: Geng Diangang

SHANDONG BINNONG TECHNOLOGY CO., LTD.
Stamp:
Date: June 02, 2022

FACTORY:

 地址: 中国山东省滨州市滨北办事处永莘路518号
 ADD: NO.518, YONGXIN ROAD, BINBEI TOWN, BINZHOU, SHANDONG, CHINA
 TEL: +86-543-5087722 FAX: +86-543-5087788
 P.C.: 256600 Website: www.binnong.com

SALES COMPANY:

 地址: 中国山东省滨州市黄河11路1111号
 ADD: NO. 1111, HUANGHE 11 ROAD, BINZHOU CITY, SHANDONG PROVINCE, CHINA
 TEL: +86-543-3368839/3367311 FAX: +86-543-3356775/3363612
 REG.DEP.: +86-543-3363985 E-mail: bns@binnong.com

APPENDIX C: CERTIFICATE OF ANALYSIS FOR REFERENCE ITEM

Dr. Ehrenstorfer

 Reference Materials for
Residue Analysis

Certificate of Analysis
ISO Guide 34 Reference Material
Product Identification

Article Code: DRE-C13725000
Article Name: Flumioxazin
Formula: C19H15FN2O4
Mol. Weight: 354.33
CAS No.: 103361-09-7

Lot Number: G140220
Expiry Date: 16.02.2023
Storage Temperature: 20°C ± 4°C

Storage and handling: The RM should be stored in the original sealed bottle at the temperature given above. After use the bottle should be tightly closed and protected from moisture and light. The expiry date is valid for original sealed bottles under recommended storage conditions only.

Purity: 99.47% (g/g)
Expanded Uncertainty U= 1.05% (g/g)

The uncertainty of this standard is calculated in accordance with the ISO Guide 34 and EURACHEM/CITAC Guide - Quantifying Uncertainty In Analytical Measurement, Second Edition. The expanded uncertainty is $U_{(exp)} = u(RM) \times k$, where k is the coverage factor at the 95% confidence level ($k=2$). Uncertainty $u(RM)$ is based on the combination of the uncertainties associated with each individual operation involved in the analysis of the product: $u(RM) = \sqrt{u(char)^2 + u(bb)^2 + u(ta)^2 + u(sts)^2}$; $u(char)$ is the uncertainty of purity determination; $u(bb)$ uncertainty of homogeneity test; $u(sts)$ uncertainty of stability test long-term; $u(sts)$ uncertainty of stability test short-term. $u(ts)$ and $u(sts)$ are not included in the calculation as the stability statement is based on real evidence opposed to simulation. Minimum sample: 1 mg is recommended as the minimal sample amount. If less material is used, it is recommended to increase the certified uncertainty by a factor of two for half sample and a factor of four for a quarter of sample. Intended use: Use this RM as calibrant for chromatography or any other analytical technique.

Analytical Data

Traceability of chromatography: To the International System of Units (SI).
Instrument: HPLC/DAD **Method Details:**
Detection: DAD **Acetonitrile:Water 4:1**
Column: ReproSil 100 C18 5 µm 250 x 3 mm
Inj.-Vol.: 10 µl
Flow: 1.0 ml/min
Ret. Time: 1.62 min

Comment

Traceability: The balances used are calibrated with weights traceable to the national standards (DKD).
 Calibrated class A glassware is used for volumetric measurements.
 Certificate Revision 1
 Purity was determined by quantitative NMR.

Identity: EA, NMR, RT, IR, UV

Certified on: 26.05.2017
Certified by: N. Müller



The LGC Labor GmbH, accredited by DAkkS as indicated by the accreditation number D-RM-19883-01 & D-PL-19883-01, has shown competence based on ISO Guide 34:2009 with relevant parts of DIN EN ISO/IEC 17025:2005 for production of certified reference materials in form of organic pure substances and in form of single and multi-component solutions of organic pure substances.

LGC Labor GmbH - Bgm.-Schlosser-Straße 6A - 86199 Augsburg - Germany
 Phone +49 821 9060880 - Fax +49 821 9060888 - augsburg.inquiry@lgcgroup.com
 The warranty for this product is limited to the purchasing price of this product.

To be continue

Data File L:\GERÄTE BACKUP\DAD4\2017\2017KW07\130217-2 2017-02-13 15-53-28\13725000.D

14.02.17
14


```

=====
Acq. Operator   : SYSTEM                      Seq. Line :   28
Acq. Instrument : LCMS                       Location  :   54
Injection Date  : 13.02.2017 21:49:12        Inj       :    1
                                           Inj Volume: 10.000 µl

Acq. Method     : C:\Chem32\1\Data\2017KW07\130217-2 2017-02-13 15-53-28\41K.M
Last changed    : 13.02.2017 15:53:29 by SYSTEM
Analysis Method : L:\GERÄTE BACKUP\DAD3\METHODS\41K.M
Last changed    : 10.11.2015 09:04:07 by DAD3_Admin
Method Info     : Acetonitrile : Water 4:1

Sample Info     : Flumioxazin
    
```

Additional Info : Peak(s) manually integrated

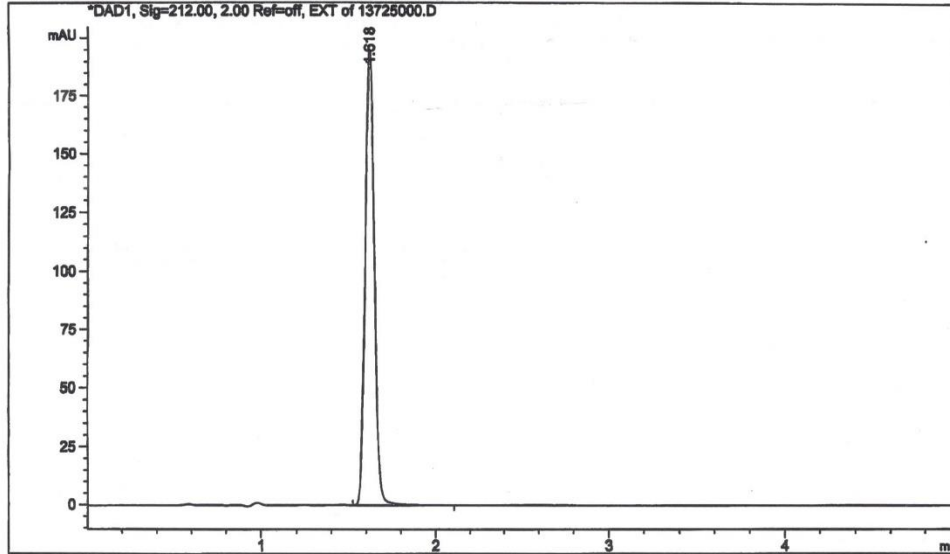

=====
Area Percent Report
=====

```

Sorted By      :      Retention Time
Multiplier    :      1.0000
Dilution      :      1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: DAD1, Sig=212.00, 2.00 Ref=off, EXT
Signal has been modified after loading from rawdata file!

Peak #	RetTime [min]	Sig	Type	Area [mAU*s]	Height [mAU]	Area %
1	1.618	1	BB	717.47504	196.52742	100.0000

Totals : 717.47504 196.52742

=====
*** End of Report ***